

FIG. 11

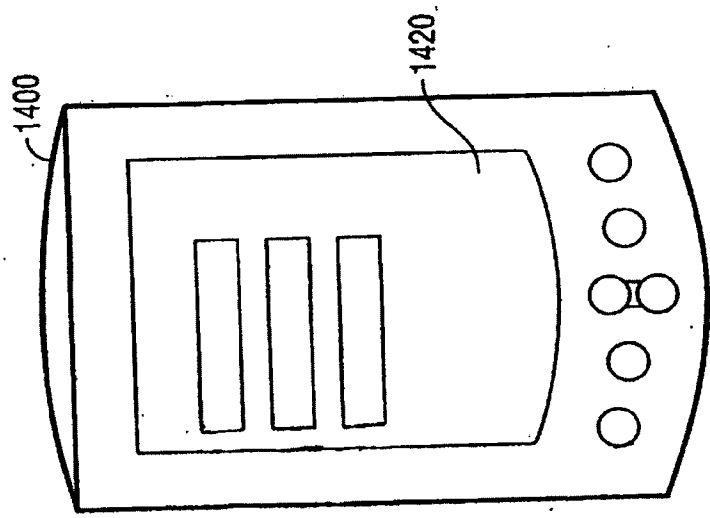


FIG. 14

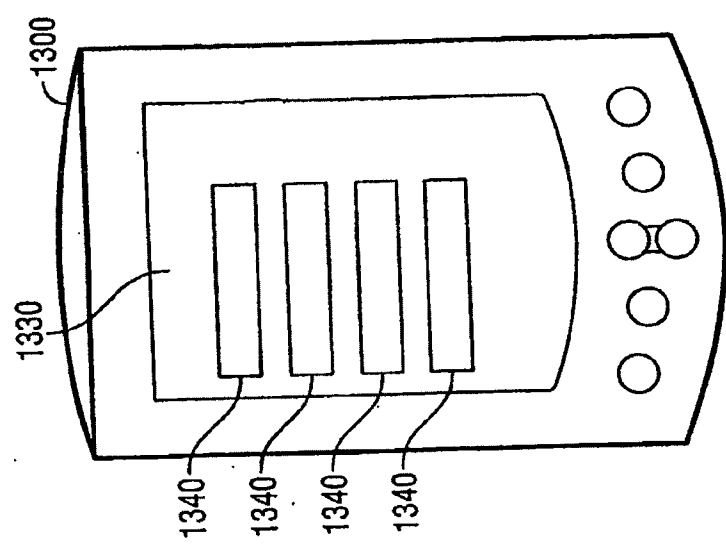


FIG. 13

4187

Nurse A, RN

Log Out

Patient, One
 Rm - Bed 101-B
 Dr. One (111)111-1111 ext. 1

Pharm & Pump Comparison

Ancel 1 g. In Dextrose, 5% 50 mL
 run at 100 mL/hr

Pharm Label	?	Pump Settings
Rate	100 mL/hr	? mL/hr

Cannot Compare.
 Press "Rate" key and COMPARE.

COMPARE

4817

FIG. 41

4087

Nurse A, RN

Log Out

Patient, One
 Rm - Bed 101-B
 Dr. One (111)111-1111 ext. 1

Pharm & Pump Comparison

Ancel 1 g. In Dextrose, 5% 50 mL
 run at 100 mL/hr

Pharm Label	≠	Pump Settings
Rate	100 mL/hr	50 mL/hr

Please Verify with PHYSICIAN Order.
 Then to accept the mismatch, press "Start" key on pump
 and then click "OK" below.
 You can also reprogram the pump and then click
 "Compare again."

OK

COMPARE

4817

FIG. 40

4825